

3D Simulation Of An Amorphous Silicon Photodiode For Particle Therapy

K. El Achi¹, E. Cortina Gil¹, A. Warnier², V. De Beco², S. Rossomme²

¹Université Catholique de Louvain, Louvain-la-Neuve, Belgium

²IBA Dosimetry, Louvain-la-Neuve, Belgium

Abstract

Proton and Radiotherapy are leading particle therapy tactics used to combat chronic and malignant cancers [1]. Ultra-high dose rate (UHDR) flash therapy is a new treatment modality that is currently being studied by several groups. The treatment delivers high doses in a short period of time (40 Gy/s) and is highly effective against tumor cells while maintaining healthy cells. Moreover, particle therapy also has radiobiological advantages compared to conventional therapy [2]. UHDR dosimetry presents a crucial challenge to detectors when performing proper quality assurance (QA) measurements. This work aims to build a high-resolution semiconductor-based 2D flat panel (FP) detector that is compatible with low-dose radiotherapy and flash proton therapy. Among semiconductor materials, amorphous Silicon (a-Si) is notable for its high radiation tolerance and ability to produce large-area pixels at low cost [3]. State-of-the-art X-ray FP detectors employ a-Si pixels coupled with a thin-film transistor (TFT) technology. On the other hand, CMOS detectors that use crystalline Silicon (c-Si) are limited by wafer size and radiation hardness but experience fast and accurate signal acquisition [4]. An in-depth study of the behavior of a-Si and c-Si under particle beams for QA will be conducted.

Focusing on a-Si and using the Semiconductor Module, COMSOL Multiphysics was employed to simulate the perspective photodiodes and understand the behavior of such technology. Starting from a simple block of thickness 1.2 μm and width $\sim 5\mu\text{m}$, the predefined built-in material Silicon in COMSOL was edited to fit the parameters of a-Si and then assigned to the block. Using the Analytical Doping Model, background acceptor doping of $N_{\text{bkg}} \sim 10^{11} \text{ cm}^{-3}$ is set to the domain. Additionally, an n-doping and p-doping layer, each with a concentration of 10^{20} cm^{-3} , were added using the Box distribution of the Analytical Doping Model, creating a 3D PIN a-Si photodiode. A square is added to the top p-layer and added as a Metallic Contact to introduce a reverse-bias voltage, and the bottom n-layer is grounded. This is represented in Figure 1. The stationary study is performed with an auxiliary sweep to sweep through different reverse-bias voltages, with the finite element discretization. Effectively, the I-V curve and electric field across the junction of the diode are resolved, as shown in Figures 2 and 3.

In addition, Garfield++ [5], a Monte Carlo (MC)-based simulation toolkit that specializes in gas and semiconductor-based detectors, was interfaced with COMSOL to perform signal and charge analysis. Using the dedicated class `Garfield::ComponentComsol()`, the mesh file and electric potential files were exported from COMSOL into Garfield++, and the exact solution of the electric field at each mesh point was used to simulate the particle track and electric signal induced on the electrodes. Figure 4 shows the current signal from irradiation normalized to a single 100 MeV proton event at different reverse-bias voltages.

COMSOL Multiphysics proves to be a very reliable and efficient toolkit to simulate the working principles of a-Si photodiodes. Further in-depth simulations will be done to build an a-Si TFT in 3D and compare all the results with an existing sample.

Keywords: Semiconductor Module, aSi TFT, Medical Dosimetry, Quality Assurance.

Reference

- [1] E. C. Halperin, "Particle therapy and treatment of cancer," *The lancet oncology*, vol. 7, no. 8, pp. 676–685, 2006.
- [2] B. Lin, D. Huang, F. Gao, et al., "Mechanisms of flash effect," *Frontiers in Oncology*, vol. 12, p. 995 612, 2022.
- [3] Ducourant, T., Wirth, T., Bacher, G., Bosset, B., Vignolle, J. M., Blanchon, D., ... & Rohr, P. (2018, March). Latest advancements in state-of-the-art aSi-based x-ray flat panel detectors. In *Medical Imaging 2018: Physics of Medical Imaging* (Vol. 10573, pp. 1498-1508). SPIE.
- [4] Job, I. D., Ganguly, A., Vernekohl, D., Weisfield, R., Muñoz, E., Zhang, J., ... & Colbeth, R. (2019, April). Comparison of CMOS and amorphous silicon detectors: determining the correct selection criteria, to optimize system performance for typical imaging tasks. In *Medical Imaging 2019: Physics of Medical Imaging* (Vol. 10948, pp. 101-112). SPIE.
- [5] H. Schindler, R. Veenhof, Garfield++ | simulation of ionisation based tracking detectors, 2018, URL <http://garfieldpp.web.cern.ch/garfieldpp/>

Figures used in the abstract

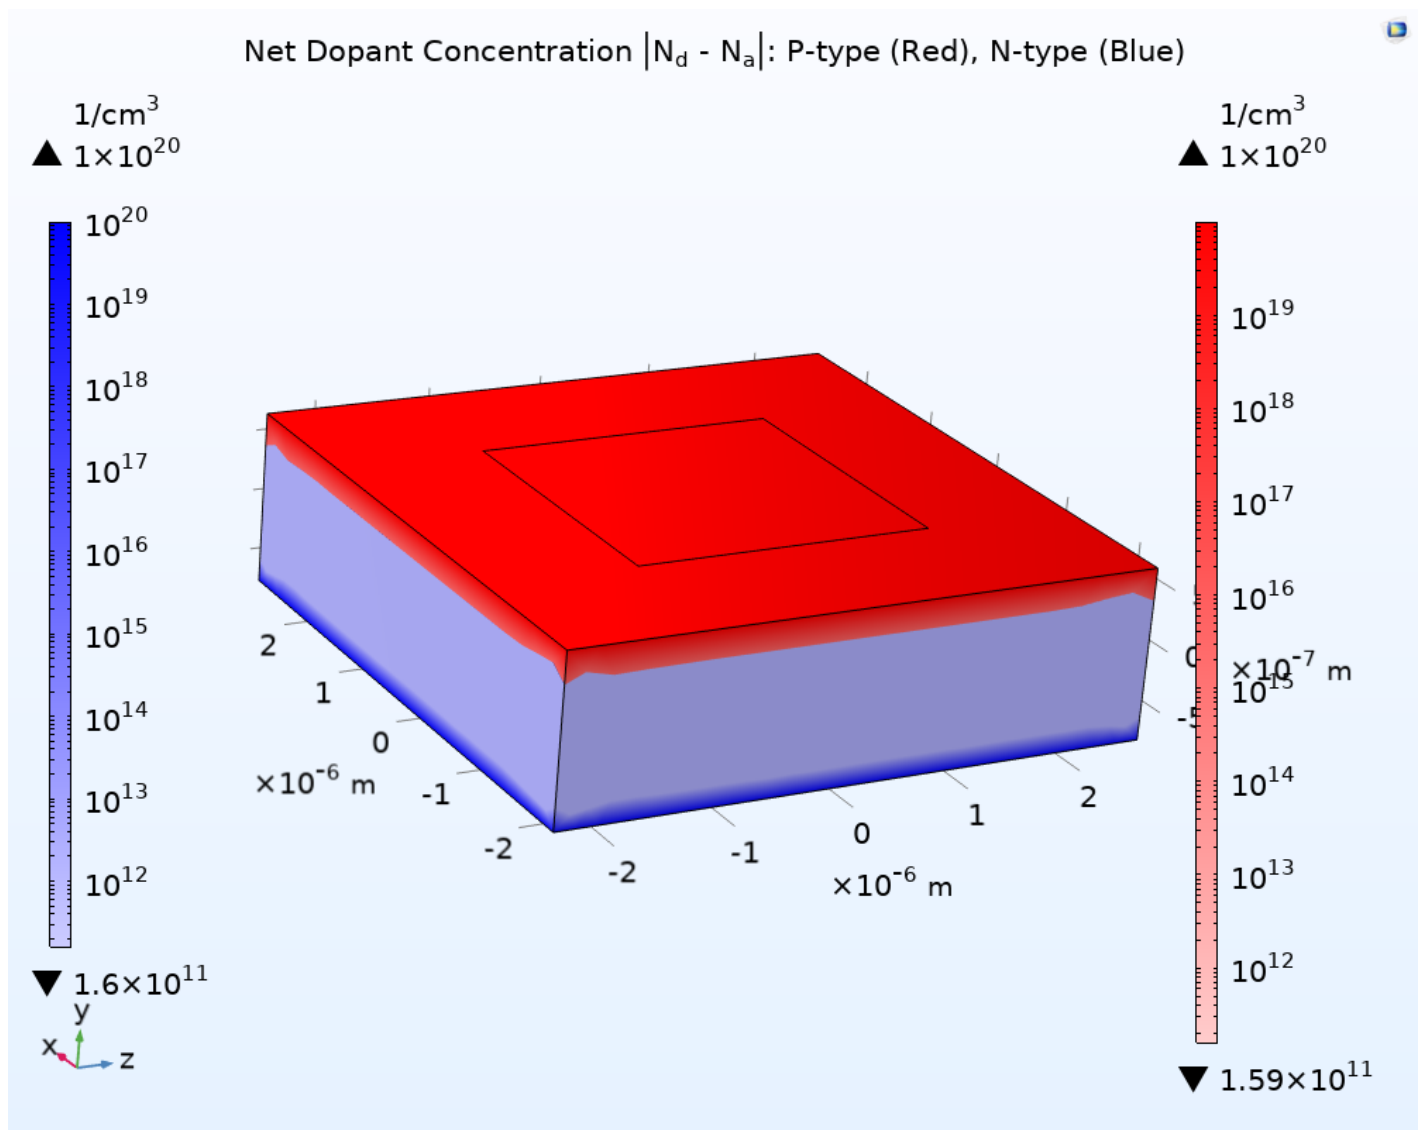


Figure 1 : Figure 1: The Net dopant concentration of a PIN diode shows the top p-doped layer and the bottom n-doped layer.

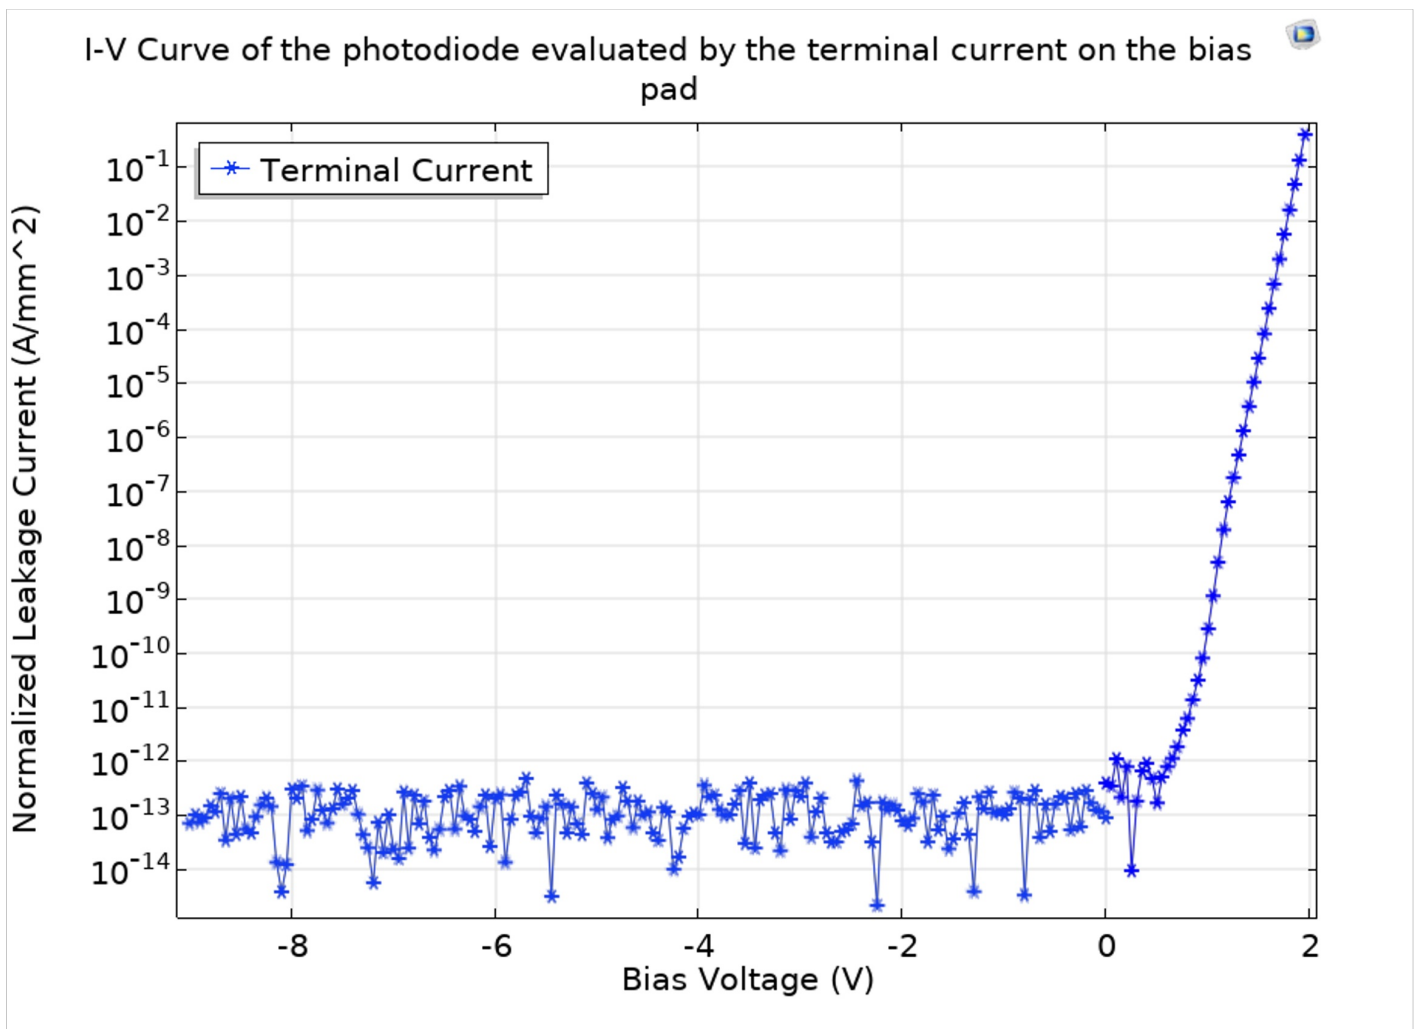


Figure 2 : Figure 2: The terminal current of the simulated PIN diode with respect to different bias voltages.

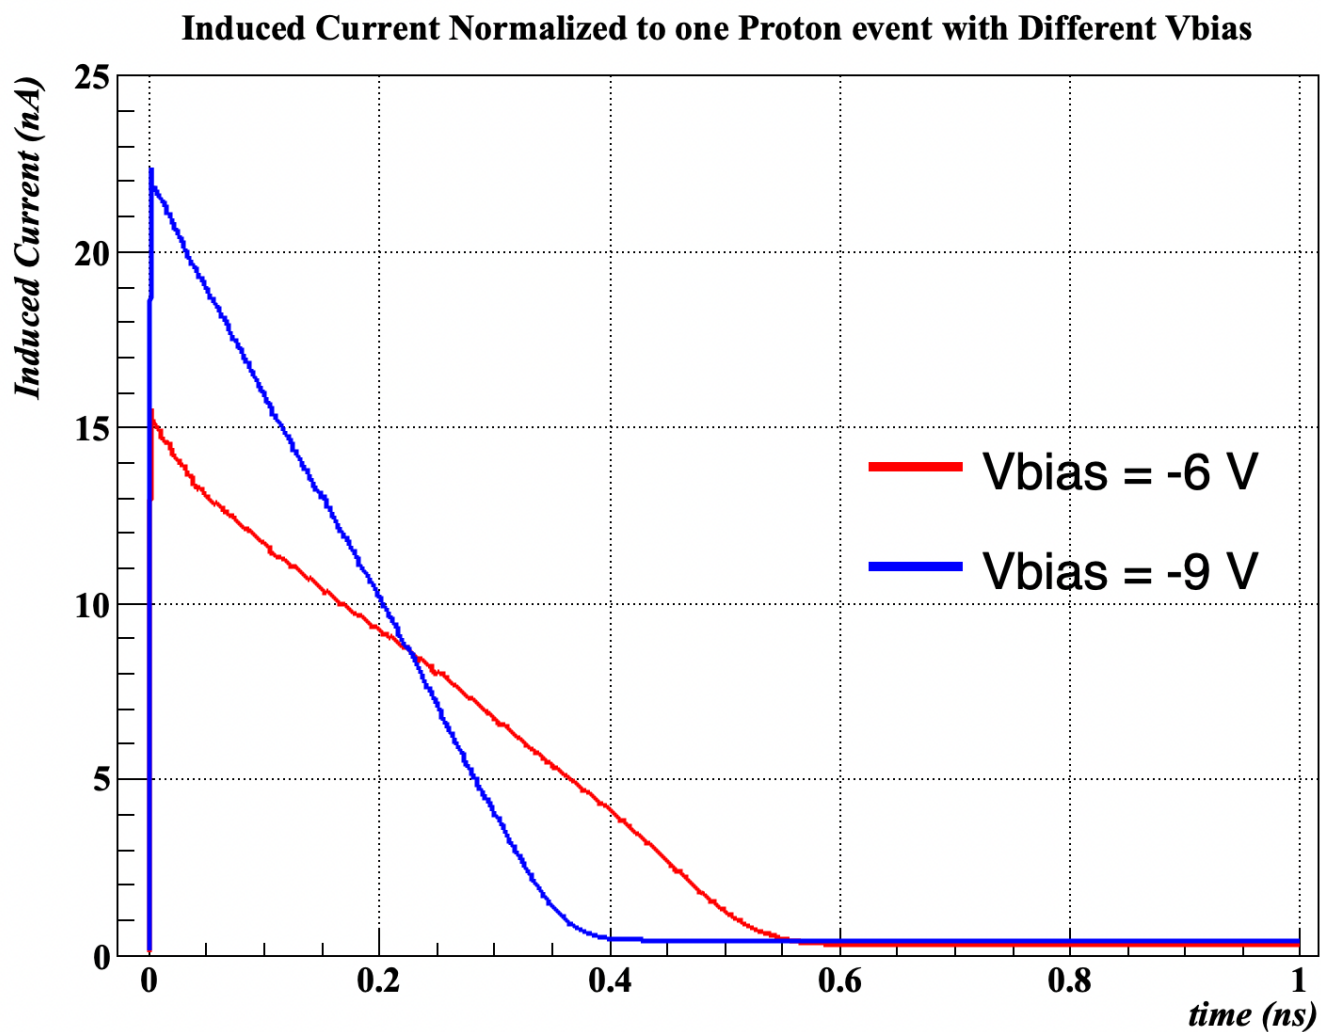


Figure 4 : Figure 4: The induced current normalized to one 100 MeV proton event at two reverse bias voltages.